


4792-29-4

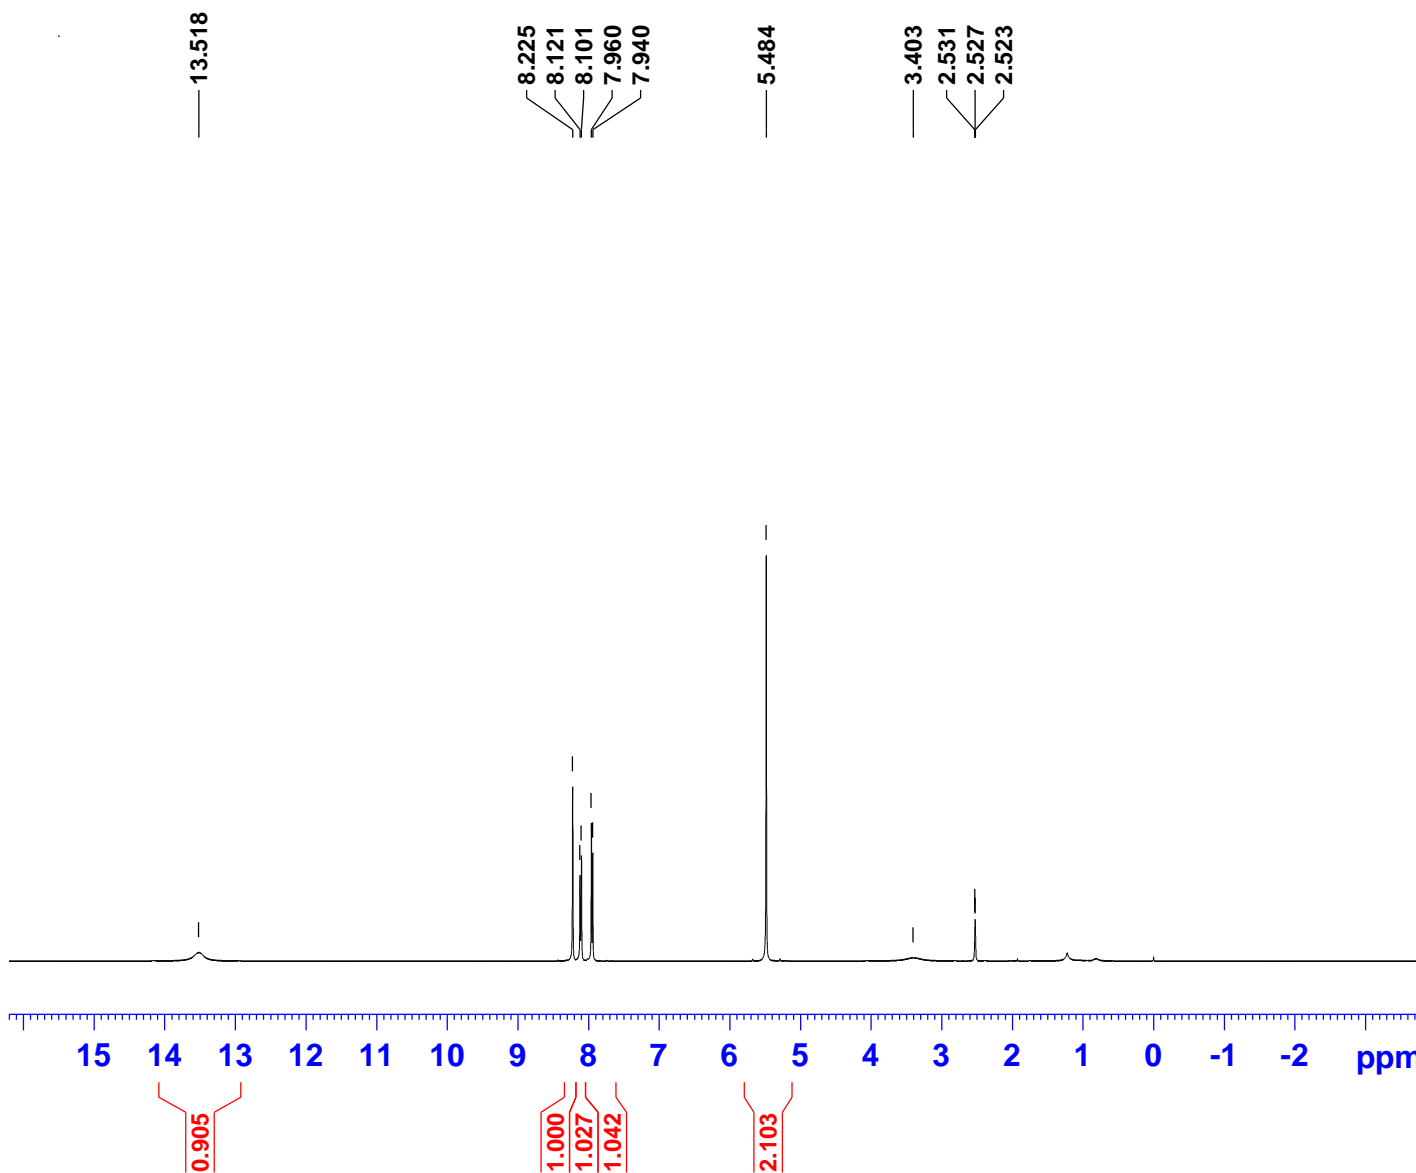

Current Data Parameters
NAME 4792-29-4
EXPNO 20
PROCNO 1

F2 - Acquisition Parameters
Date_ 20190819
Time 17.50 h
INSTRUM spect
PROBHD Z116098_0564 (
PULPROG zg30
TD 65536
SOLVENT DMSO
NS 16
DS 2
SWH 8012.820 Hz
FIDRES 0.244532 Hz
AQ 4.0894465 sec
RG 77.67
DW 62.400 usec
DE 6.50 usec
TE 300.0 K
D1 1.00000000 sec
TD0 1
SFO1 400.1324708 MHz
NUC1 1H
P1 9.93 usec
PLW1 14.56099987 W

F2 - Processing parameters
SI 65536
SF 400.1299924 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00