


3.391
3.374
3.358
2.516
2.501
2.484
1.421
1.404
1.388
1.372
1.339
1.322
1.305
1.290
1.275
1.267
1.260
1.250
1.109

Current Data Parameters
 NAME 4048-33-3-20211008-HNMR
 EXPNO 1
 PROCNO 1

F2 - Acquisition Parameters
 Date_ 20211008
 Time 12.55 h
 INSTRUM spect
 PROBHD Z108618_0072 (
 PULPROG zg30
 TD 32768
 SOLVENT DMSO
 NS 8
 DS 0
 SWH 8012.820 Hz
 FIDRES 0.489064 Hz
 AQ 2.0447233 sec
 RG 101
 DW 62.400 usec
 DE 6.50 usec
 TE 297.7 K
 D1 1.00000000 sec
 TD0 1
 SFO1 400.1424709 MHz
 NUC1 1H
 P1 10.00 usec
 PLW1 35.00000000 W

F2 - Processing parameters
 SI 65536
 SF 400.1400000 MHz
 WDW EM
 SSB 0
 LB 0.30 Hz
 GB 0
 PC 1.00

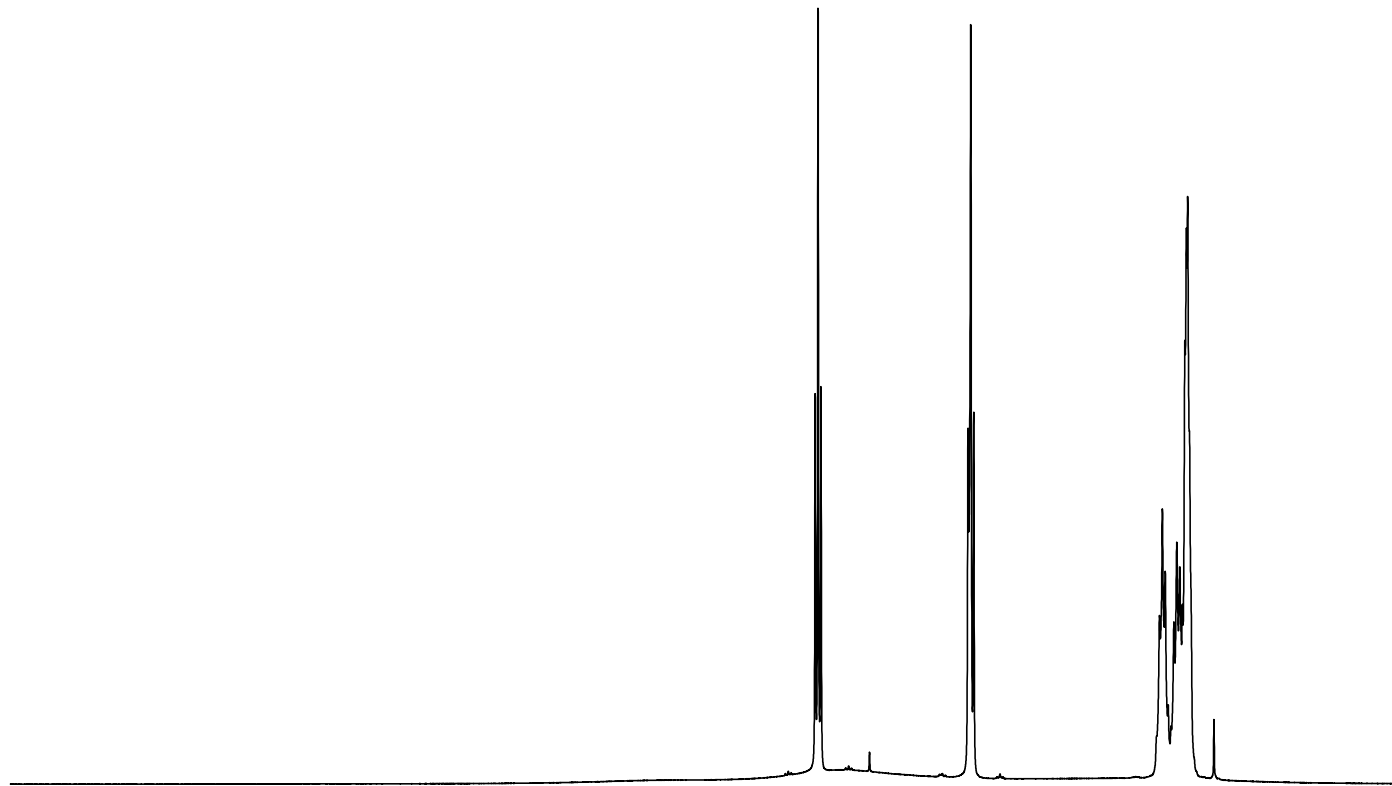

7.5 7.0 6.5 6.0 5.5 5.0 4.5 4.0 3.5 3.0 2.5 2.0 1.5 1.0 ppm

Scale: 0.4324 ppm/cm, 173.0 Hz/cm

2.006
2.638
2.000
5.874
0.188