


3.391
3.374
3.358
2.516
2.501
2.484
1.421
1.404
1.388
1.372
1.339
1.322
1.305
1.290
1.275
1.267
1.260
1.250
1.109

Current Data Parameters
NAME 4048-33-3-20211008-HNMR
EXPNO 1
PROCNO 1

F2 - Acquisition Parameters
Date_ 20211008
Time 12.55 h
INSTRUM spect
PROBHD Z108618_0072 (
PULPROG zg30
TD 32768
SOLVENT DMSO
NS 8
DS 0
SWH 8012.820 Hz
FIDRES 0.489064 Hz
AQ 2.0447233 sec
RG 101
DW 62.400 usec
DE 6.50 usec
TE 297.7 K
D1 1.00000000 sec
TD0 1
SFO1 400.1424709 MHz
NUC1 1H
P1 10.00 usec
PLW1 35.00000000 W

F2 - Processing parameters
SI 65536
SF 400.1400000 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

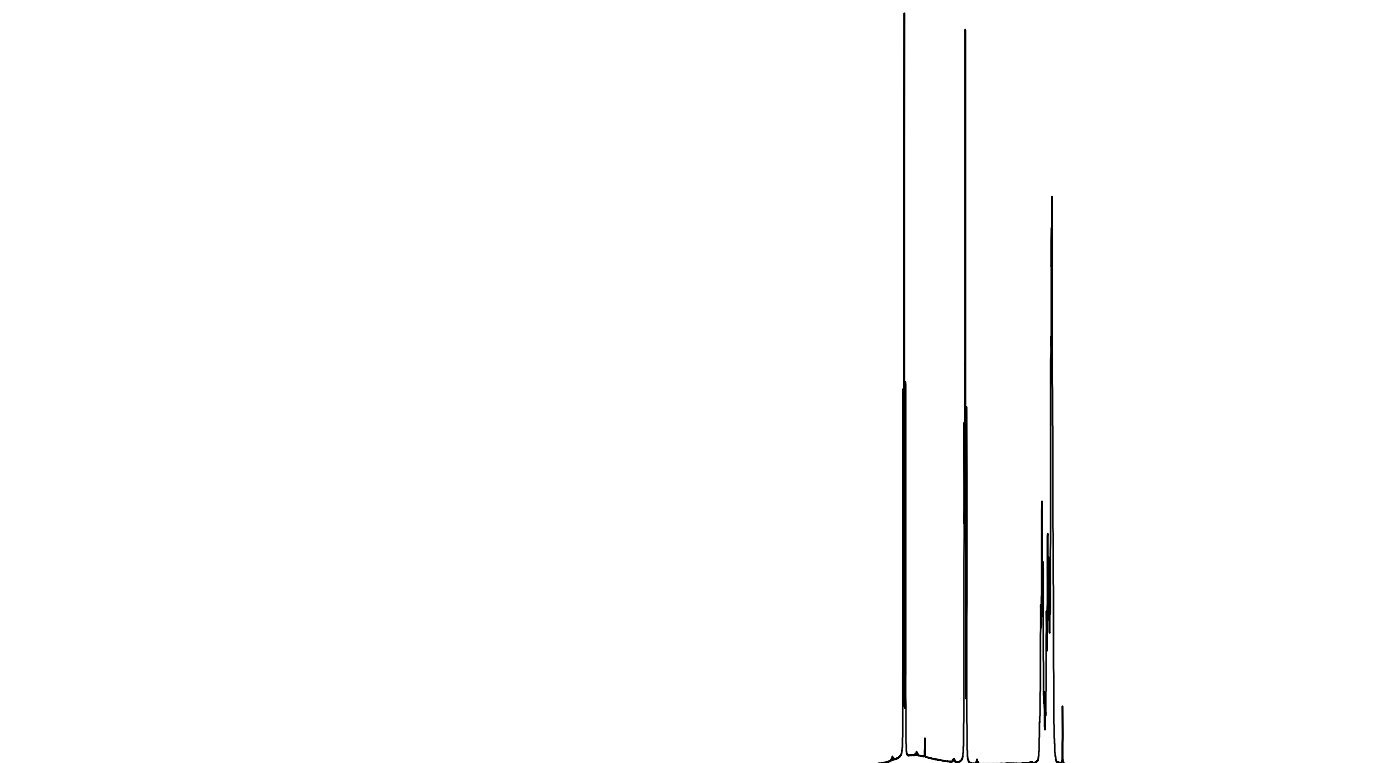

15 14 13 12 11 10 9 8 7 6 5 4 3 2 1 0 -1 -2 ppm

Scale: 1.082 ppm/cm, 433.1 Hz/cm

2.006
2.638
2.000
5.874
0.188